

10-05-00

A

10/04/00

JC760 U.S. PRO 10/04/00

LAW OFFICES

FREILICH, HORNBAKER & ROSEN
PROFESSIONAL CORPORATION

ARTHUR FREILICH
BERT D. HORNBAKER
LEON D. ROSEN
TIMOTHY T. TYSON

10960 WILSHIRE BOULEVARD, SUITE 1220
LOS ANGELES, CA 90024-3702
TEL. (310) 477-0578 • FAX (310) 473-9277
E-MAIL l.rosen@prodigy.net

SAN FERNANDO VALLEY OFFICE
9045 CORBIN AVENUE, SUITE 260
NORTHridge, CA 91324
TEL (818) 678-6408 • FAX (818) 678-6411

PATENTS, TRADEMARKS & RELATED INTELLECTUAL PROPERTY MATTERS

PATENT TRANSMITTAL FORM

DOCKET: 20/168

JC930 U.S. PRO 09/678616

10/04/00

Hon. Commissioner of Patents

Express Mail Label EL080585710US

Date of Deposit October 04, 2000

Washington, D.C. 20231

Enclosed for filing is a patent application entitled CHEST COMPRESSOR by Max Harry Weil, Joe Bisera, Clayton Young, and Wanchun Tang.

This is a _____ of application Serial No. _____ filed _____.

☒ Enclosed is an Assignment for recordation with a Recordation Form Cover Sheet.

☒ Enclosed is a verified statement to establish small entity status.

☒ Enclosed are 3 sheets of drawings.

☐ Enclosed is a Prior Art Disclosure (Information Disclosure Citation).

☐ Enclosed is a Priority Document Submittal and Priority Document _____ appl. _____.

☒ Enclosed is Declaration for Patent Application.

☒ Enclosed is a postcard for stamping upon receipt and return.

The filing fee has been calculated as shown below:

ITEM	CLAIMS		SMALL ENTITY		NON SM. ENTITY	
	# Filed	# Extra	Rate	Fee	Rate	Fee
1. Basic Fee:				355		710
2. Total Claims:	<u>12</u>	- 20 =	x 9 =		x 18 =	
3. Independent Claims:	<u>4</u>	- 3 = <u>1</u>	x 40 =	<u>40</u>	x 80 =	
4. Multiple Dependent Claim		=				
FILING FEE				<u>=\$395</u>		<u>=\$</u>

☒ Our check for \$435.00 to cover the following items is enclosed:

<input checked="" type="checkbox"/> Filing Fee	\$ <u>395.00</u>
<input checked="" type="checkbox"/> Recordation Fee (\$40)	\$ <u>40.00</u>
TOTAL:	\$ <u>435.00</u>

Throughout the prosecution of this application the Commissioner of Patents and Trademarks is authorized to charge any additional fees which may be required, or credit any overpayment to Account No. 06-1985.

Leon D. Rosen
Attorney for Applicant(s)
Reg. No. 21,077

I hereby certify that this paper or fee is being deposited with the United States Postal service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 on the date indicated above and is addressed to the Commissioner of Patents, Washington, D.C. 20231.

Label No. EL080585710US
Date of Deposit October 04, 2000

Leon D. Rosen

cc: Mr. Joe Bisera

Applicant or Patentee: Max Harry Weil, Joe Bisera, Clayton Young, and Wanchun Tang

Docket No 20/168

Serial or Patent No:

Filed or Issued:

For: CHEST COMPRESSOR

VERIFIED STATEMENT (DECLARATION) CLAIMING SMALL ENTITY STATUS
(37 CFR 1.9(f) and 1.27(c)) - SMALL BUSINESS CONCERN

I hereby declare that I am

- ☐ the owner of the small business concern identified below:
☒ an official of the small business concern empowered to act on behalf of the concern identified below.

NAME OF CONCERN:

The Institute of Critical Care Medicine

ADDRESS OF CONCERN

1695 N. Sunrise Way, Palm Springs, CA 92262

I hereby declare that the above identified small business concern qualifies as a small business concern as defined in 13 CFR 121.3-18, and reproduced in 37 CFR 1.9(d), for purposes of paying reduced fees under section 41(a) and (b) of Title 35, United States Code, in that the number of employees of the concern, including those of its affiliates, does not exceed 500 persons. For purposes of this statement. (1) the number of employees of the business concern is the average over the previous fiscal year of the concern of the persons employed on a full-time, part-time or temporary basis during each of the pay periods of the fiscal year, and (2) concerns are affiliates of each other when either, directly or indirectly, one concern controls or has the power to control the other, or a third party or parties controls or has the power to control both.

I hereby declare that rights under contract or law have been conveyed to and remain with the small business concern identified above with regard to the invention, entitled: CHEST COMPRESSOR

by Inventor(s) Max Harry Weil, Joe Bisera, Clayton Young, and Wanchun Tang
described in

- ☒ the specification filed herewith
☐ application serial no. _____, filed _____.
☐ patent no. _____, issued _____.

If the rights held by the above identified small business concern are not exclusive, each individual, concern or organization having rights to the invention is listed below* and no rights to the invention are held by any person, other than the inventor, who could not qualify as a small business concern under 37 CFR 1.9(d) or by any concern which would not qualify as a small business concern under 37 CFR 1.9(d) or a nonprofit organization under 37 CFR 1.9(e). *NOTE: Separate verified statements are required from each named person, concern or organization having rights to the invention averring to their status as small entities. (37 CFR 1.27)

FULL NAME

ADDRESS

☐ INDIVIDUAL ☐ SMALL BUSINESS CONCERN ☐ NONPROFIT ORGANIZATION

FULL NAME

ADDRESS

☐ INDIVIDUAL ☐ SMALL BUSINESS CONCERN ☐ NONPROFIT ORGANIZATION

I acknowledge the duty to file, in this application or patent, notification of any change in status resulting in loss of entitlement to small entity status prior to paying, or at the time of paying, the earliest of the issue fee or any maintenance fee due after the date on which status as a small entity is no longer appropriate. (37 CFR 1.28(b))

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under section 1001 of Title 18 of the United States Code, and that such willful false statements may jeopardize the validity of the application, any patent issuing thereon, or any patent to which this verified statement is directed.

NAME OF PERSON SIGNING:

Max Harry Weil

TITLE OF PERSON OTHER THAN OWNER:

President

ADDRESS OF PERSON SIGNING:

1695 N. Sunrise Way, Palm Springs, CA 92262

SIGNATURE

Date

10/04/00
09/678616
Jc930 U.S. PTO

CHEST COMPRESSOR

ABSTRACT OF THE DISCLOSURE

Apparatus for compressing the chest of a patient to stimulate blood circulation, includes a torso wrap (32) that has a back portion (40) lying at the back of the patient's chest and a front portion (42) lying at the front of the patient's chest, and includes a compressor assembly with an actuator (16) having a pressing member (12) that can apply a series of force pulses to the sternum of the patient to stimulate blood circulation. The actuator is energized by pressured fluid, with a controlled pressured fluid source (20) connected by an elongated flexible hose (24) to the actuator so the pressured fluid source and a control (22) can lie on the ground and only the actuator lies on the torso wrap. The actuator includes a cylinder (66) and a plurality of telescoping piston parts (64, 66) to provide a long stroke in an actuator of small height. A stabilizer (150) that limits tilt of the actuator from the vertical, includes a saucer-shaped member that presses against the front of the patient.

BACKGROUND OF THE INVENTION

Low systemic perfusion is caused by several forms of circulatory shock, including hemorrhage, sepsis, and cardiac arrest, all of which cause large system-wide harm to vital organs. A first mode of damage results from the sudden decrease in oxygen delivery to cells, while a second mode of damage results from the inability to remove cellular waste products such as CO₂.

Stimulation of circulation is commonly accomplished by applying pressure pulses to the chest. This can be accomplished by placing a torso wrap around the patient, and attaching a chest compressor to the front of the torso wrap. The actuator applies downward pressure pulses to the patient's chest while the torso wrap holds down the actuator.

In order for a chest compressor system to be widely used, it must be compact and easily attached to the patient. In some cases, a rescuer may be positioned so it is most convenient for him/her to attach the torso wrap by slipping the part with the chest compressor under the patient. A chest compressor of small height aids in such attachment. It is important that the chest compressor lie with its axis normal to the patient's chest and not tilt by more than several degrees from that orientation. A chest compressor system with a compact and light weight actuator for actually compressing the chest, would be of value.

SUMMARY OF THE INVENTION

In accordance with one embodiment of the present invention, an apparatus is provided for applying compressions to the chest of a patient to stimulate circulation, which is compact, of light weight, and reliable. The apparatus includes an energizable compressor assembly with a pressing member that can apply a series of pulses to the chest of the patient, and a

torso wrap that wraps around the back of the patient's torso so the patient's torso is sandwiched between the compressor and the back portion of the torso wrap. The compressor assembly includes an actuator that is energized by pressured fluid such as pressured gas and that is coupled to the torso wrap.

5

The compressor assembly also includes a fluid source and control that are coupled through an elongated flexible tube to the actuator so the pressure source and control can lie on the ground beside the patient. The control includes a valve that briefly opens periodically to send pulses of air to the actuator to cause the pressing member to be depressed in pulses.

10

The actuator can include a cylinder connected to the torso wrap and a piston that slides vertically within the cylinder. The piston includes a plurality of piston parts that telescope to provide a long stroke in an actuator of small height.

15

A stabilizer includes a plurality of leg portions with inner ends connected to the actuator and outer ends that press against the person's chest to prevent tilt of the actuator. The stabilizer can be formed by a saucer-shaped member of greater diameter than the pressing member. The torso wrap can include an eyelet attached to one side of the stabilizer and a strap that extends from the opposite side of the stabilizer and around the patient, with an end portion of the strap threaded through the eyelet and tightened, with Velcro pads on the strap holding the strap in its tightened position.

20

The novel features of the invention are set forth with particularity in the appended claims. The invention will be best understood from the following description when read in conjunction with the accompanying drawings.

25

/

//

///

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 illustrates a patient who is reclined on a floor and who is being treated for dangerously low profusion, such as may exist for a patient undergoing a heart attack.

5

Fig. 2 is a sectional view of the compressor assembly of Fig. 1.

Fig. 3 is an isometric view of apparatus for applying compressions to the patient's sternum to increase circulation, and for also compressing the patient's torso so as to encourage respiration.

10

DESCRIPTION OF THE PREFERRED EMBODIMENTS

Fig. 1 illustrates a patient P who has a dangerously low blood circulation such as might occur in a heart attack. An apparatus 10 of the invention includes a compression assembly 14 with a pressing member 12 having a diameter of about three inches, which can be forcefully pushed down against the sternum S of the patient's chest in a series of pulses, to stimulate the heart of the patient. For an adult male patient, the pressing member 12 can press down with a maximum force of about 100 to 120 lbs., in pulses spaced by perhaps ½ to 1 second apart. This mimics the chest compressions applied in CPR (cardiopulmonary resuscitation).

15

20

The compression assembly 14 includes an actuator 16 that forces down the pressing member 12 in pulses, a pressure source 20 that supplies pressured air for energizing the actuator, and a control 22 that controls the application of pressure to the actuator. An elongated flexible tube 24 connects the remote part 30 of the compressor assembly that lies on the ground, to the actuator 16 that lies over the patient's chest.

25

The apparatus 10 includes a torso wrap 32 which includes a belt or band 34 that extends largely around the upper torso of the patient. The band has a

back portion 40 that lies at the back Q of the patient and a front portion 42 that lies at the front of the patient. A first end 50 of the band is coupled to one side of the actuator 16 while an opposite second end 52 of the band is coupled to the opposite side of the actuator. The opposite sides of the actuator are spaced in a lateral direction N which extends in left L and right R directions of the patient. When the actuator 16 is energized, it pushes the pressing member 12 in a downward or backward B direction, while the rest of the actuator 16 tends to move in a forward F direction relative to the patient. During such downward pulses of the pressure member 12, the actuator 16 and opposite sides 50, 52 of the band front portion move forwardly, with such movement resisted by the back portion of the band.

Fig. 2 shows details of the compressor assembly 14, including the actuator 16 and the remote portion 30. The actuator 16 includes a cylinder 60 and a piston 62 largely within the cylinder. The particular piston 62 includes two piston parts 64, 66. A cap 70 covers the top of the cylinder, while the pressing member 12 is mounted on the bottom of the inner piston part 66. When pressured air is supplied through an inlet 72 to the inside of the cylinder, such pressured air presses downward against the inner piston part 66, especially its large area bottom inner surface 74. This compresses the patient's chest. The maximum downward travel of the pressing member 12 and inner piston part 66 are shown at 12A and 66A. At that position, shoulders 80, 82 on the piston parts engage corresponding shoulders 84, 86, one on the cylinder and one on the outer piston part. The maximum downward stroke 90 can exceed the actuator height 92.

The pressure source 20 is shown as including a pressured fluid container 100 and a regulator 102. The pressured fluid container 100 may, for example, include a large carbon dioxide cartridge that contains gas under high

pressure that may exceed 1,000 psi. The regulator 102 allows only a much lower pressure such as 80 psi to pass through it, with an adjuster 104 provided to vary the applied pressure. The control 30 includes an electronic control box 110 and a valve 112. The control box 110 supplies current pulses to a solenoid 114 of the valve to withdraw a valve member 116 against the force of a spring 118. The withdrawn valve member allows pressured air to flow through a passage 120 and through the flexible elongated tube 24 into the inlet 72 of the actuator.

The tube 24 has a large diameter inside 130, such as 3/8 inch (0.375 inch), so that a high pressure pulse is rapidly transmitted through the tube to the actuator. Actually, the maximum pressure in the cylinder is only about one-fourth of the pressure output of the regulator, depending on tube and cylinder size, etc. If a small diameter tube (e.g. 0.1 inch I.D.) were used, then rapid pulses of air of sufficient volume could not be delivered from the regulator (at 80 psi) through a tube of over 20 cm length so as to sufficiently rapidly depress the pressing member 12 for adequate CPR. The tube 24 has a minimum length to rapidly pass gas pulses through it, although a length of at least about 1.5 feet is generally necessary. A safety valve 132 allows the escape of gas of high pressure (e.g. over 20 psi) in the cylinder. Gas rapidly leaks out of the piston through an exit 134.

It would, instead, be possible to provide a pressured gas storage compartment that was fixed to the actuator 16 to supply pressured pulses through a valve to the actuator. However, this would increase the height and weight of the apparatus that was fixed to the torso wrap. Instead, applicant minimizes the weight, and especially the height of the actuator 16 by providing controlled air pulses through a remote portion 30 that rests on the ground. A quick connect coupling 120 enables a fitting 122 at the outer end of the tube 24

to be rapidly attached to a fitting 124 on the actuator for rapid connection.

5 The actuator has a vertical axis 140 which should be maintained within about 5° from a vertical direction when the patient's chest location 182 that is being compressed lies in a horizontal plane. The band 34 shown in Fig. 1 has a width W such as 2 inches for compact storage and easy deployment, and provides some resistance to tilt of the actuator axis. However, even if the flexible band were much wider, it would not apply much resistance to actuator tilt. To prevent such tilt, applicant provides a stabilizer 150. The stabilizer has at least two leg portions 152, 154, one lying in an upward direction T from the actuator and the other 154 lying downward D from the actuator. This prevents tilt of the actuator about a lateral axis N, with the tightened bands providing some resistance to tilt about a perpendicular horizontal axis. Preferably, applicant provides many leg portions spaced about the axis. The particular stabilizer 150 is in the form of a saucer. As shown in Fig. 2, the stabilizer has one or more outer ends 160 spaced a radial distance 162 from the axis 140 that is considerably more than the radius 164 of the pressing member 12. With at least three and preferably at least four locations angularly spaced about the axis 140, lying against or very close to the location 182 of the chest that is being compressed, applicant prevents more than a few degrees of tilt of the actuator. The radius of the stabilizer outer ends is preferably more than that of the pressing member but not more than three times as great.

20 To install the apparatus 10 (Fig. 1) on a person, a rescue worker slips an end portion 170 of the band under the person's back, and then threads the tip of the band end through an eyelet 172 on a short band part 176. The person pulls on the band end part 176 that has passed through the eyelet until the band is tight on the person. Then, the band end part 176 is pressed against another band end part 178, with both parts 176, 178 having Velcro

(hook and loop type fasteners) pads to prevent loosening of the belt. As also shown in applicant's Fig. 2, the band ends 50, 52 can be fastened by rivets 180, 182 to the stabilizer 150. The stabilizer is fastened by rivets 184 to a flange on the cylinder of the actuator.

5 It is possible for the stabilizer to be formed by a plurality of feet or legs 190 that can be pivoted up (or horizontally) out of the way for storage and later pivoted down and locked in the down position. However, applicant prefers to use the saucer-like stabilizer, shown for simplicity.

10 When mounting the chest compressor assembly on the patient, applicant prefers to place the center of the pressing member 12, at its axis, about two inches above (in direction T) the sternum notch (which lies at the middle and bottom of the sternum) and preferably about two inches to the left L of the center line C of the patient's torso. This places the pressing member where it is most likely to stimulate the heart. However, compression applied at
15 nearby locations on the sternum such as at the center line of the sternum, will work almost as well. It should be noted that it is possible to use a rigid torso wrap, which needs to be only of C shape to encircle about 180° of the torso instead of 360°. However, applicant prefers the flexible band for easy storage and low weight.

20 In many cases, it is desirable to induce breathing in the patient as well as stimulating the patient's heart. Fig. 3 shows an apparatus 220 that includes a first portion 222 for stimulating a patient's heart and a second portion 226 for stimulating breathing. The apparatus 222 is similar to that of Figs. 1 and 2, with a wide flexible band 224 that holds an actuator 16. The band has two
25 straps 230, 232 to provide tight band portions at the top and bottom of the wide band. The second portion 226 includes a band 240 that extends in about a full circle (at least 270°) around the person's middle torso, and includes a pair of

actuators 242, 244 for controllably tightening the band to compress the middle torso. The actuators 242, 244 are energized by compressed gas pulses delivered over a line 250 from a control 252. The chest compressor actuator 16 is energized by compressed gas pulses delivered through a line 254 that is also connected to the control. A graph 260 shows a sequence of seven chest compression pulses 162 applied during a period of about 5 seconds to the chest compressor actuator. Pulses of the same characteristics are applied by the apparatus of Figs. 1 and 2. Another graph 264 shows pulses 266 applied to the breathing actuators 242, 244 to compress the middle chest of the patient about four times during a period of about 6 seconds. It is noted that it is generally desirable to start breathing of the patient by blowing air directly into the mouth of the patient, but many persons will not place their mouth next to the mouth of another person, especially a stranger, and the breathing helping apparatus 226 is a reasonable alternative.

Fig. 4 shows one of the chest compression pulses 262 applied as gas along the tube and applied as pressure to the patient's chest. The pulse has a rapid rate of increase at 270 and a smaller rate of decrease at 272, with the rate at 272 being less than half the rate at 270.

Although the patient is usually placed in a reclined position, with his back on a horizontal floor or stretcher, the back of the patient may not lie on a horizontal surface, as where it lies on a staircase, although the back portion of the torso wrap still presses against the back of the patient.

Thus, the invention provides an apparatus for applying compressions to the chest of a patient to stimulate blood circulation and a method for installing and operating it, which includes a compact and relatively light weight apparatus to be installed on the patient. This is accomplished by using an actuator energized by pulses of pressured gas, with the pressured gas supplied through

an elongated flexible tube from a remote portion of a compression assembly that normally lies on a floor beside the patient. An actuator of small height but long maximum stroke length can be provided by a piston comprising a plurality of piston parts that telescope in one another, and a pressing member attached to the innermost piston part. The orientation of the actuator on the patient is closely controlled by a stabilizer having a larger diameter than that of the pressing member, and which can press against the patient's chest around the actuator to avoid large tilt of the actuator. The torso wrap is preferably in the form of a flexible band, with one side of the band that extends from one side of the actuator forming an eyelet, and the other side of the band which wraps around the patient being pulled through the eyelet to tighten the band on the patient, and with the tightened end portion fixed by Velcro pads.

Although particular embodiments of the invention have been described and illustrated herein, it is recognized that modifications and variations may readily occur to those skilled in the art, and consequently, it is intended that the claims be interpreted to cover such modifications and equivalents.

WHAT IS CLAIMED IS

1. Apparatus for applying compressions to the chest of a patient to stimulate blood circulation, comprising:

an energizable compressor assembly which includes an actuator that is energized by pressured fluid and that has a pressing member that is pushed against the patient's chest;

a torso wrap that couples to said actuator and that wraps to the back of the patient, so downward forces of the piston against the patient's chest are withstood by upward forces applied to the patient's back;

said compressor assembly including a pressured fluid source, an elongated flexible hose with an inner end coupled to said fluid source and an outer end coupled to said actuator, and a control assembly with a controlled valve that connects said pressure source to said hose in pulses that travel through said hose and cause said piston to be depressed in pulses, to thereby minimize the volume and weight of the combination of torso wrap and actuator carried by the torso wrap.

2. The apparatus described in claim 1 wherein:

said actuator includes a cylinder and a piston, with said piston including a plurality of telescoping piston parts including a first piston part that fits closely in said cylinder and a second piston part that fits closely in said first piston part.

3. The apparatus described in claim 1 wherein:

said apparatus is constructed to increase the pressure of fluid at a first rapid rate in said actuator and then decrease the pressure in said actuator at a

second rate that is less than half said first rate.

4. The apparatus described in claim 1 wherein said actuator has a vertical axis, and including:

a stabilizer that includes a plurality of leg portions that each has an inner end connected to said actuator and an outer end that is positioned to press against the front of the patient, with said outer ends spaced about said axis to minimize tilt of the actuator vertical axis.

5. The apparatus described in claim 1 wherein:

said actuator has laterally opposite sides, and said torso wrap includes an eyelet coupled to a first of said actuator sides and a band coupled to the other of said actuator sides, with said band having an end portion with an end part that is threadable through said eyelet and with said belt end portion having a pair of Velcro pads that attach the end part to the rest of said belt end portion.

6. Apparatus for applying compressions to the chest of a patient to stimulate blood circulation, comprising:

an energizable compressor assembly which includes an actuator with a cylinder and a piston, and a source of pressured fluid;

a torso wrap that couples to said actuator and that wraps to the back of the patient, so downward forces of the piston against the patient's chest are withstood by upward forces applied to the patient's back;

said actuator includes a cylinder coupled to said torso wrap and a plurality of telescoping piston parts including a first piston part that fits closely

10 in said cylinder and a second piston part that fits closely in said first piston part, with at least said second piston part exposed to pressured fluid in said cylinder, and including a pressing member on a lower end of said second piston part for pressing against the patient's chest.

7. The apparatus described in claim 6 wherein:

5 said compressor assembly includes an elongated flexible hose with an inner end coupled to said fluid source and an outer end coupled to said actuator, and a control assembly with a control valve that connects said pressure source to said hose in pulses that travel through said hose to said actuator.

8. Apparatus for applying compressions to the chest of a patient to stimulate blood circulation, comprising:

5 an energizable compressor assembly which includes an actuator that has a vertical axis and a pressing member for pressing against the patient;

5 a torso wrap that couples to said actuator and that wraps to the back of the patient, so downward forces of the pressing member against the patient's chest are withstood by upward forces applied to the patient's back;

10 a stabilizer that includes a plurality of leg portions that each has an inner end connected to said actuator and an outer end that is positioned to press against the front of the patient, with said outer ends spaced about said axis to minimize tilt of the actuator with respect to the patient's front.

9. The apparatus described in claim 8 wherein:

said outer ends of said stabilizer leg portions are spaced further from said axis than any part of said pressing member that presses against the

patient's chest.

10. The apparatus described in claim 8 wherein:

said stabilizer comprises a saucer-shaped element with a center portion fixed to said actuator and a radially outer portion that rests substantially against the patient's chest.

11. A method for establishing chest compression equipment on a patient, comprising:

placing a combination of a torso wrap and a pressured-fluid energized actuator on the patient, with the torso wrap having a portion lying against the back of the patient and with the actuator attached to on the torso wrap and having a piston lying against the front of the patient;


placing a pressured fluid source and control assembly on a floor, and coupling the pressured fluid source and control assembly through a hose to the actuator, whereby to minimize the weight and volume of the combination of torso wrap and actuator that must be placed on the patient.

12. The method described in claim 11 wherein:

said control assembly includes a valve that couples said pressure source to said tube; and including

opening and closing said valve periodically to transmit pressure pulses through said hose, while allowing the escape of the fluid in said actuator at least between the transmittal of pressure pulses.

FIG. 1

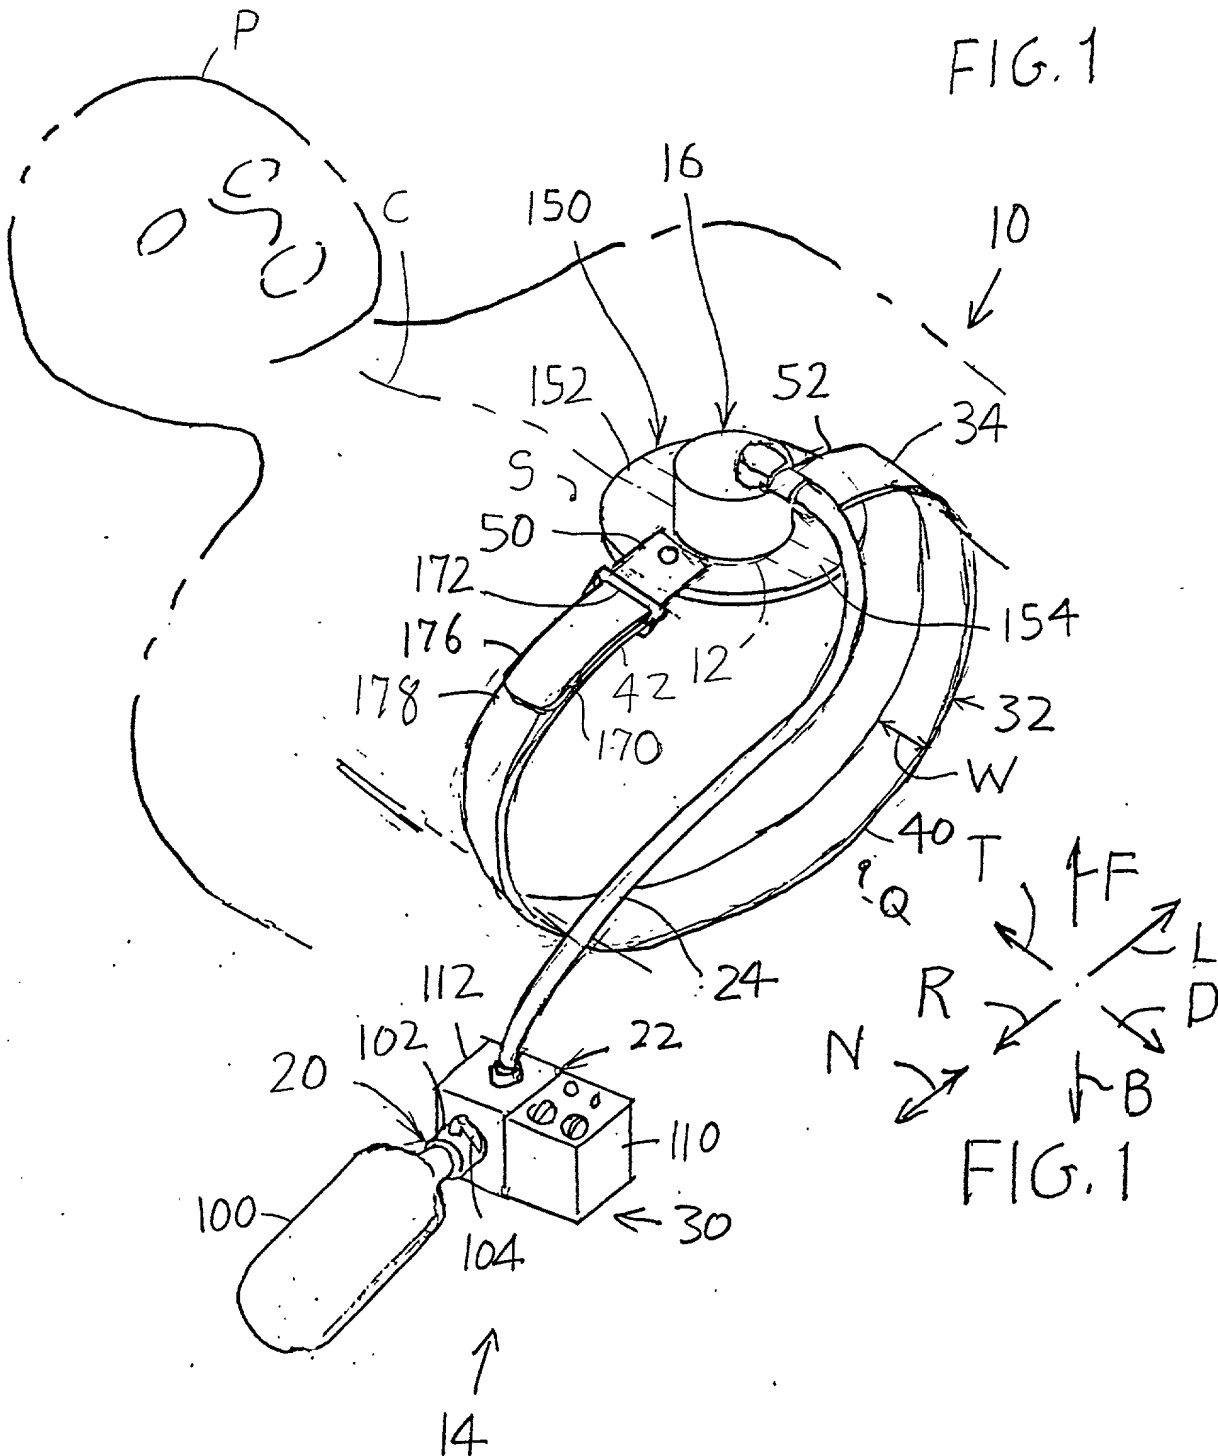

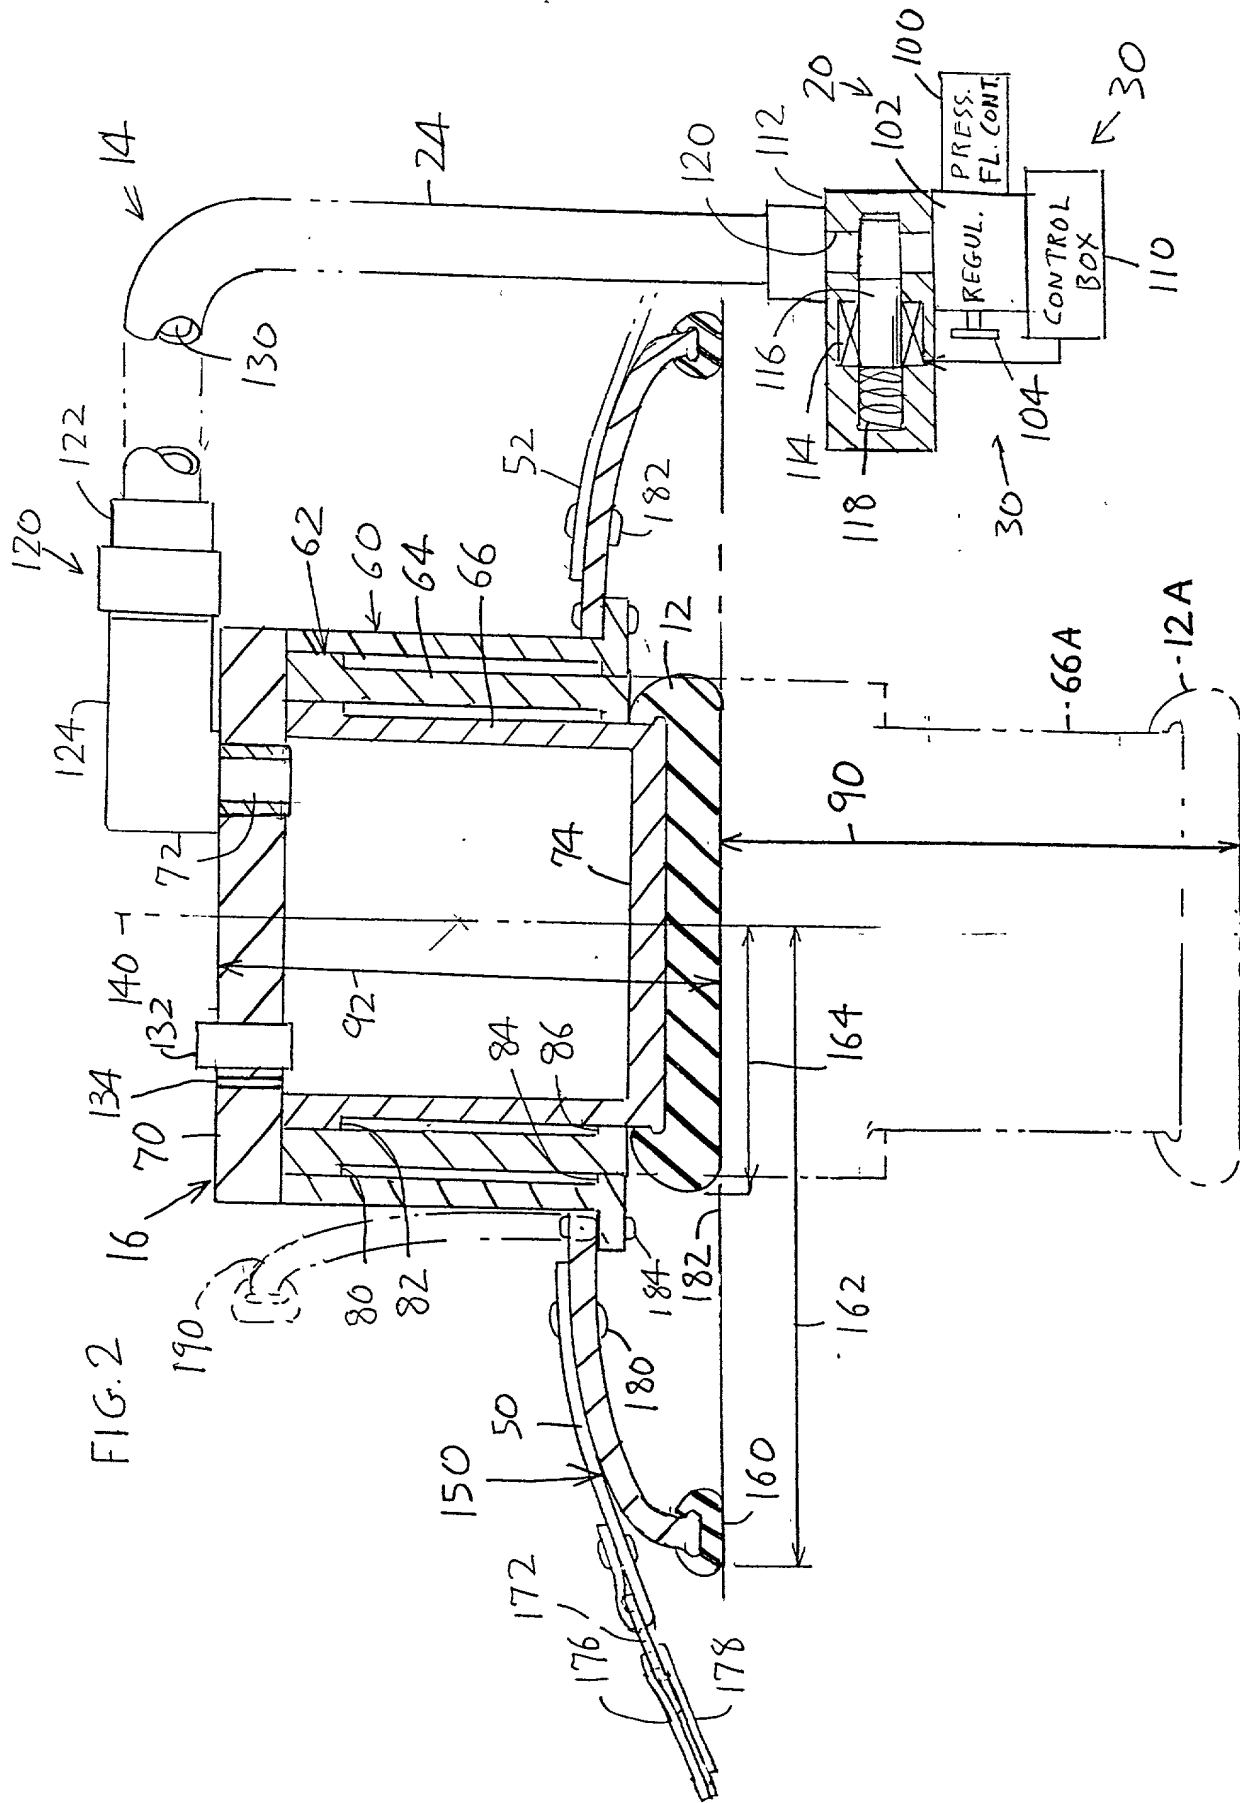


FIG. 3


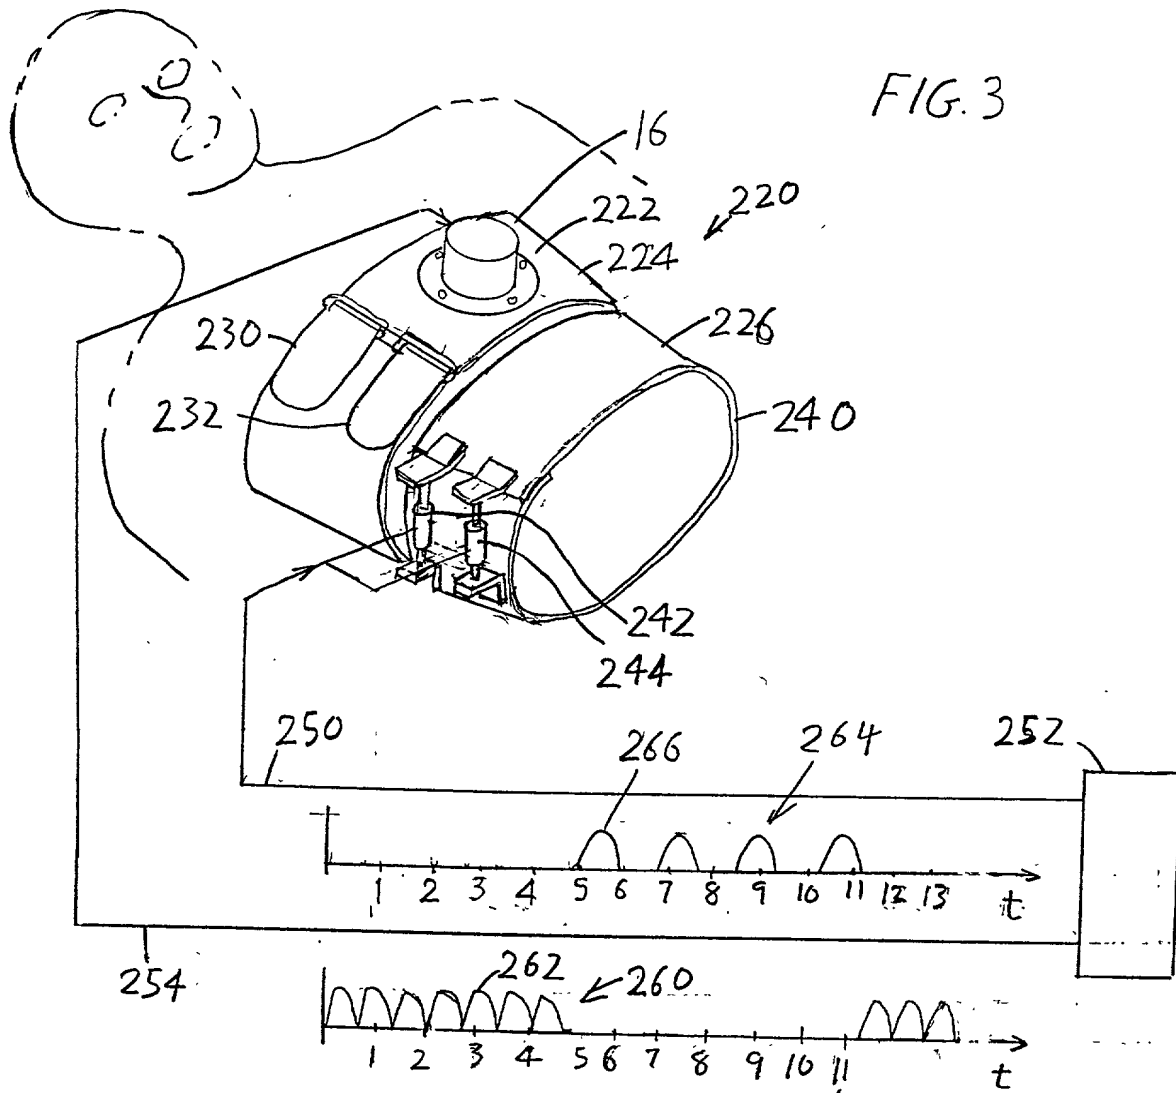


FIG. 4

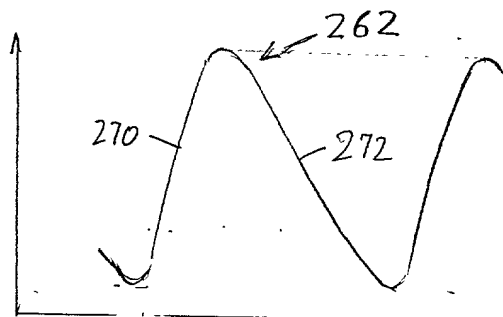

DECLARATION FOR PATENT APPLICATION

As a below named inventor, I hereby declare that:
My residence, post office address and citizenship are as stated below.

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled CHEST COMPRESSOR the specification of which X is attached hereto.

 was filed on as Application Serial No.
and was amended on (if applicable).

I hereby state that I have reviewed and understand the contents of the above-identified specification, including the claims, as amended by any amendment referred to above. I acknowledge the duty to disclose information which is material to the examination of this application in accordance with Title 37, Code of Federal Regulations, Section 1.56(a),

I hereby claim foreign priority benefits under Title 35, United States Code, §119 of any foreign application(s) for patent or inventor's certificate listed below and have also identified below any foreign application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed:

Number	Country	Date Filed	Yes	No

I hereby claim the benefits under Title 35, United States Code, §119(e) of any United States provisional application listed below:

Provisional Application Number Date Filed

I hereby claim the benefit under Title 35, United States Code, §120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code, 112, I acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, §1.56(a) which occurred between the filing date of the prior application and the national or PCT international filing date of this application:

Appl. Ser. No.	Filing Date	Status-patented, pending, abandoned

I hereby appoint the following attorney(s) to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith:

Leon D. Rosen, Reg. No. 21,077; Timothy T. Tyson, Reg. No. 28,915; Arthur Freilich, Reg. No. 19,281; Robert D. Hornbaker, Reg. No. 19,965

Address all telephone calls to: Leon D. Rosen

(310) 477-0578

Address all correspondence to:

LEON D. ROSEN

FREILICH, HORNBAKER & ROSEN

10960 Wilshire Blvd., Suite 1220

Los Angeles, CA 90024

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

Full name of sole or first inventor Max Harry Weil

Inventor's Signature [Signature]

Date Sep 29, 2000

Residence 3810 S. Mission Hills Road, #303, Northbrook, IL 60062

Citizenship USA

Post Office Address SAME

Full name of second inventor Joe Bisera

Inventor's Signature [Signature]

Date Sep 29, 2000

Residence 1534 Anacapa Drive, Camarillo, CA 93010

Citizenship USA

Post Office Address SAME

Full name of third inventor Clayton Young

Inventor's Signature [Signature]

Date 10/2/00

Residence 14593 Birch St. San Leandro CA 94579

Citizenship USA

Post Office Address SAME

Full name of fourth inventor Manchun Tang

Inventor's Signature [Signature]

Date 9/29/00

Residence 40456 Periwinkle Court, Palm Desert, CA 92660

Citizenship USA

Post Office Address SAME